


Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_6 - Detector 1)

|   | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%] | Height [%] | W05 [min] |
|---|-------------------|-------------|-------------|----------|------------|-----------|
| 1 | 20.492            | 238.919     | 2.779       | 93.4     | 86.2       | 0.14      |
| 2 | 21.172            | 16.892      | 0.444       | 6.6      | 13.8       | 1.06      |
|   | Total             | 255.812     | 3.222       | 100.0    | 100.0      |           |

Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_6 - Detector 2)

|   | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%] | Height [%] | W05 [min] |
|---|-------------------|-------------|-------------|----------|------------|-----------|
| 1 | 3.384             | 6410.000    | 1069.241    | 95.4     | 99.8       | 0.10      |
| 2 | 19.552            | 311.279     | 4.069       | 4.6      | 0.4        | 1.15      |
|   | Total             | 6721.279    | 1073.310    | 100.0    | 100.0      |           |

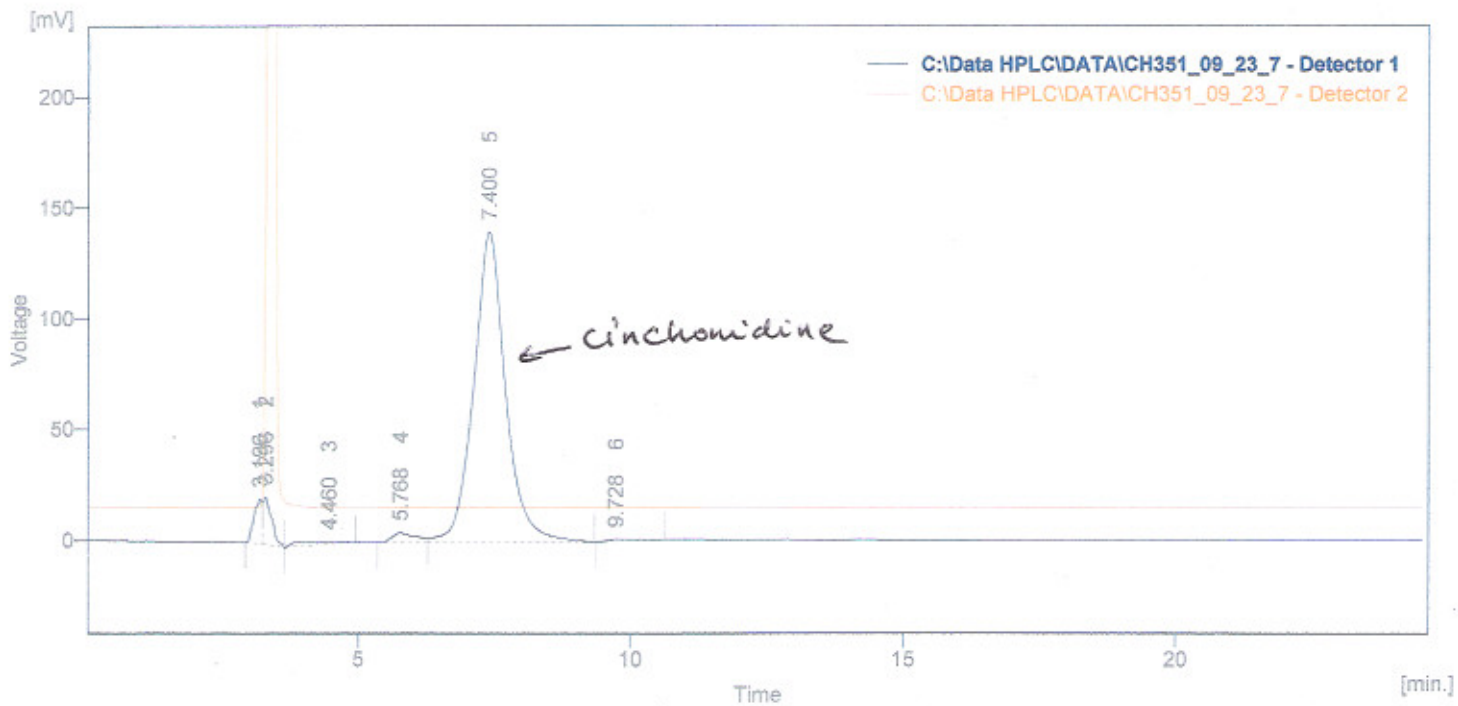


Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_7 - Detector 1)

|   | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%] | Height [%] | W05 [min] |
|---|-------------------|-------------|-------------|----------|------------|-----------|
| 1 | 3.196             | 201.579     | 20.186      | 3.2      | 10.8       | 0.17      |
| 2 | 3.296             | 242.238     | 21.511      | 3.8      | 11.5       | 0.19      |
| 3 | 4.460             | 76.376      | 1.133       | 1.2      | 0.6        | 1.14      |
| 4 | 5.768             | 119.242     | 4.078       | 1.9      | 2.2        | 0.55      |
| 5 | 7.400             | 5890.678    | 139.552     | 89.6     | 74.5       | 0.59      |
| 6 | 9.728             | 22.943      | 0.737       | 0.4      | 0.4        | 0.98      |
|   | Total             | 6353.056    | 187.186     | 100.0    | 100.0      |           |

Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_7 - Detector 2)

|   | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%] | Height [%] | W05 [min] |
|---|-------------------|-------------|-------------|----------|------------|-----------|
| 1 | 3.444             | 11125.442   | 1069.162    | 100.0    | 100.0      | 0.17      |
|   | Total             | 11125.442   | 1069.162    | 100.0    | 100.0      |           |

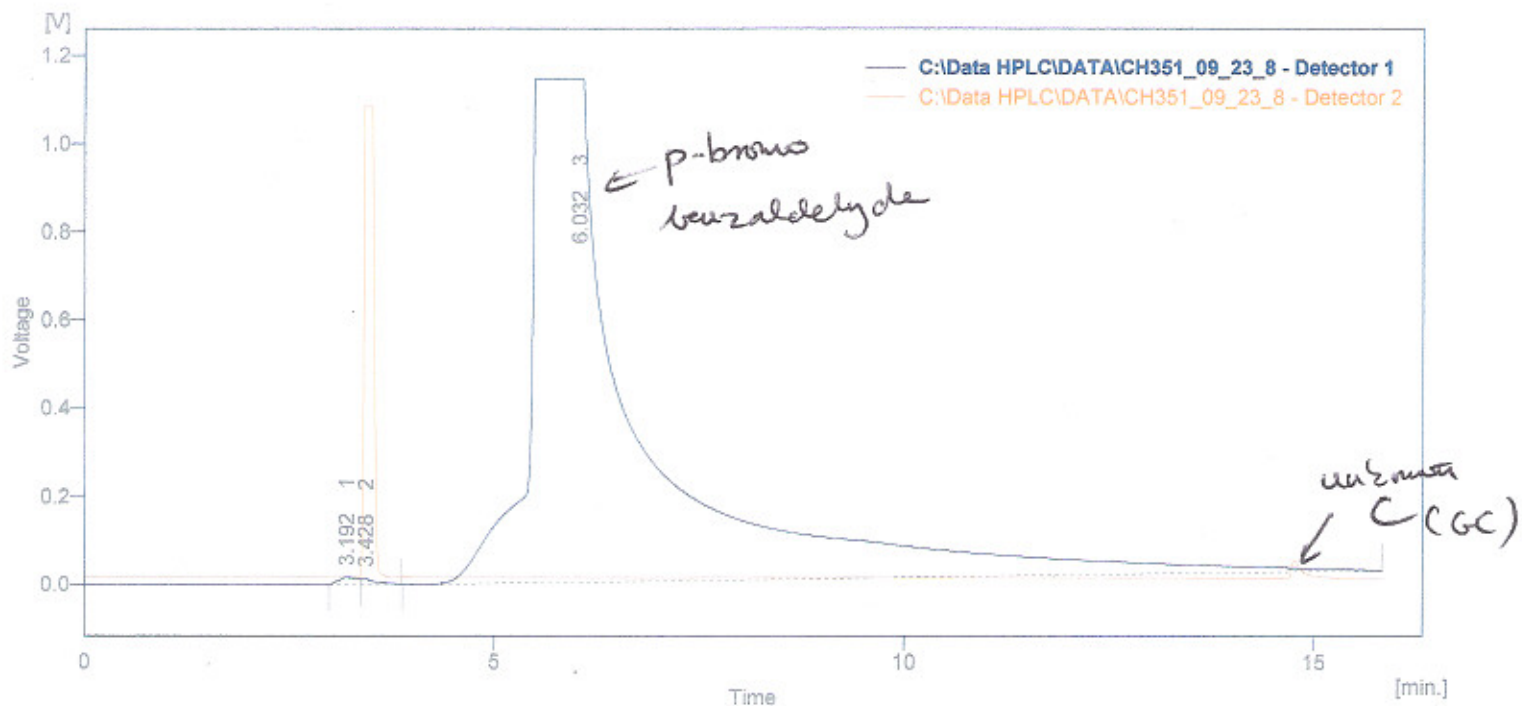


Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_8 - Detector 1)

|   | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%] | Height [%] | W05 [min] |
|---|-------------------|-------------|-------------|----------|------------|-----------|
| 1 | 3.192             | 239.876     | 15.168      | 0.2      | 1.3        | 0.28      |
| 2 | 3.428             | 163.427     | 12.887      | 0.2      | 1.1        | 0.17      |
| 3 | 6.032             | 108177.624  | 1140.502    | 99.6     | 97.6       | 0.88      |
|   | Total             | 108580.927  | 1168.358    | 100.0    | 100.0      |           |

Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_8 - Detector 2)

|   | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%]  | Height [%] | W05 [min] |
|---|-------------------|-------------|-------------|-----------|------------|-----------|
| 1 | 3.300             | 2.759       | 1.245       | 2.943e-02 | 0.1        | 0.04      |
| 2 | 3.496             | 9002.612    | 1069.180    | 96.0      | 96.5       | 0.14      |
| 3 | 14.760            | 389.649     | 37.900      | 3.9       | 3.4        | 0.13      |
|   | Total             | 9375.020    | 1108.295    | 100.0     | 100.0      |           |

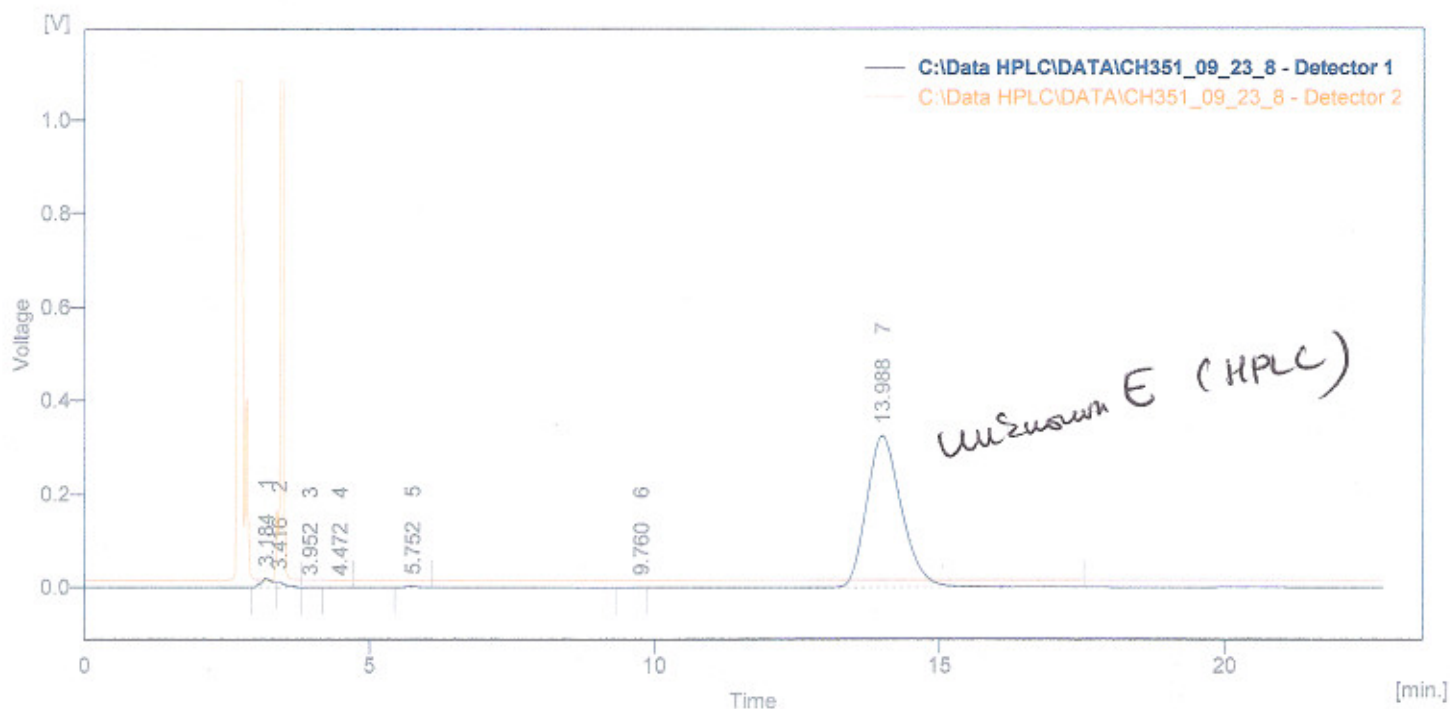


Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_8 - Detector 1)

|   | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%] | Height [%] | W05 [min] |
|---|-------------------|-------------|-------------|----------|------------|-----------|
| 1 | 3.184             | 287.203     | 19.883      | 2.0      | 5.5        | 0.28      |
| 2 | 3.416             | 144.322     | 12.692      | 1.0      | 3.5        | 0.14      |
| 3 | 3.952             | 20.790      | 1.365       | 0.1      | 0.4        | 0.31      |
| 4 | 4.472             | 15.021      | 0.544       | 0.1      | 0.2        | 0.50      |
| 5 | 5.752             | 33.363      | 1.931       | 0.2      | 0.5        | 0.28      |
| 6 | 9.760             | 17.636      | 1.197       | 0.1      | 0.3        | 0.22      |
| 7 | 13.988            | 14041.165   | 324.374     | 96.4     | 89.6       | 0.66      |
|   | Total             | 14559.501   | 361.987     | 100.0    | 100.0      |           |

Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_8 - Detector 2)

|   | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%] | Height [%] | W05 [min] |
|---|-------------------|-------------|-------------|----------|------------|-----------|
| 1 | 2.724             | 8944.015    | 1069.201    | 63.3     | 46.8       | 0.12      |
| 2 | 3.376             | 345.836     | 148.410     | 2.4      | 6.5        | 0.04      |
| 3 | 3.464             | 4834.202    | 1069.103    | 34.2     | 46.8       | 0.07      |
|   | Total             | 14124.054   | 2286.714    | 100.0    | 100.0      |           |

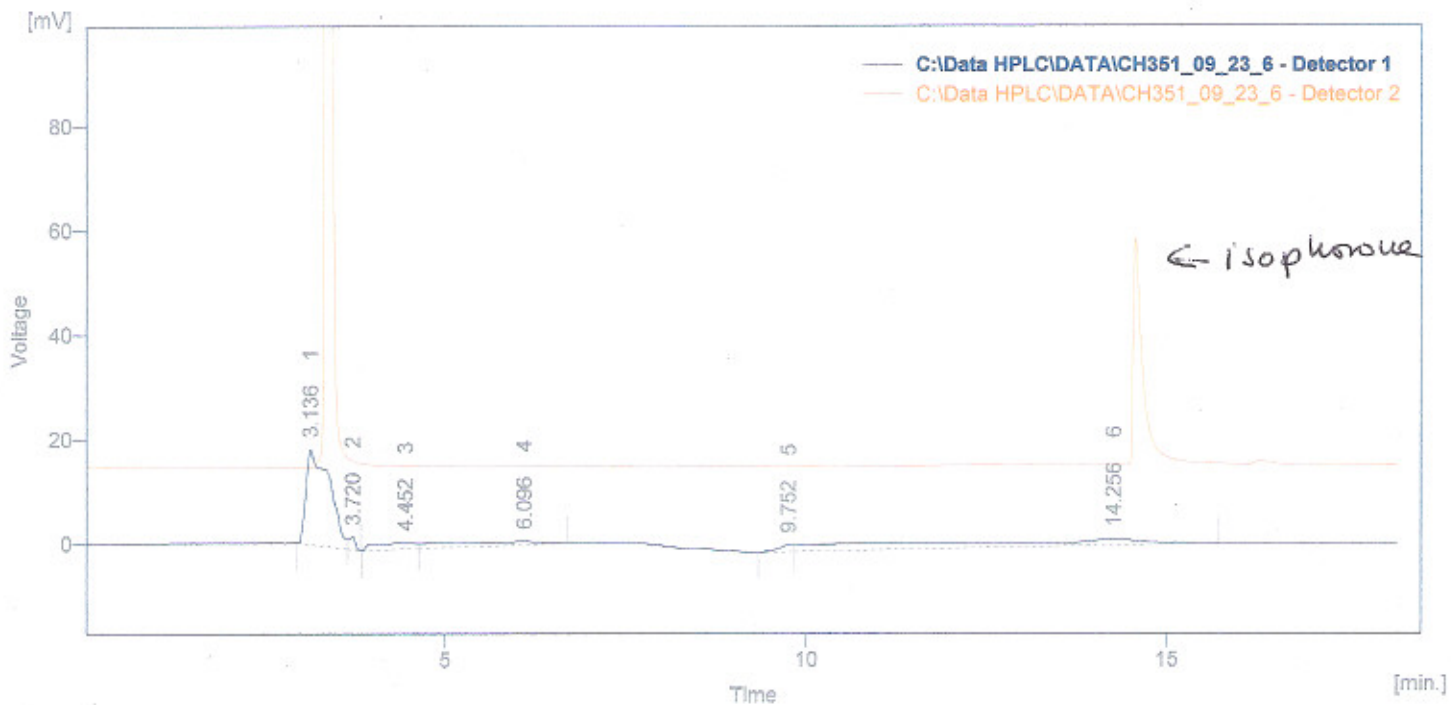


Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_6 - Detector 1)

|   | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%] | Height [%] | W05 [min] |
|---|-------------------|-------------|-------------|----------|------------|-----------|
| 1 | 3.136             | 414.919     | 18.253      | 48.5     | 72.8       | 0.39      |
| 2 | 3.720             | 16.021      | 2.436       | 1.9      | 9.7        | 0.11      |
| 3 | 4.452             | 48.843      | 1.219       | 5.7      | 4.9        | 0.73      |
| 4 | 6.096             | 71.863      | 0.729       | 8.4      | 2.9        | 0.44      |
| 5 | 9.752             | 17.761      | 1.267       | 2.1      | 5.1        | 0.21      |
| 6 | 14.256            | 286.510     | 1.169       | 33.5     | 4.7        | 0.86      |
|   | Total             | 855.718     | 25.072      | 100.0    | 100.0      |           |

Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_6 - Detector 2)

|   | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%] | Height [%] | W05 [min] |
|---|-------------------|-------------|-------------|----------|------------|-----------|
| 1 | 3.404             | 6814.679    | 1069.112    | 93.5     | 96.0       | 0.10      |
| 2 | 14.560            | 457.988     | 43.418      | 6.3      | 3.9        | 0.13      |
| 3 | 16.284            | 14.709      | 0.944       | 0.2      | 0.1        | 0.20      |
|   | Total             | 7287.356    | 1113.473    | 100.0    | 100.0      |           |

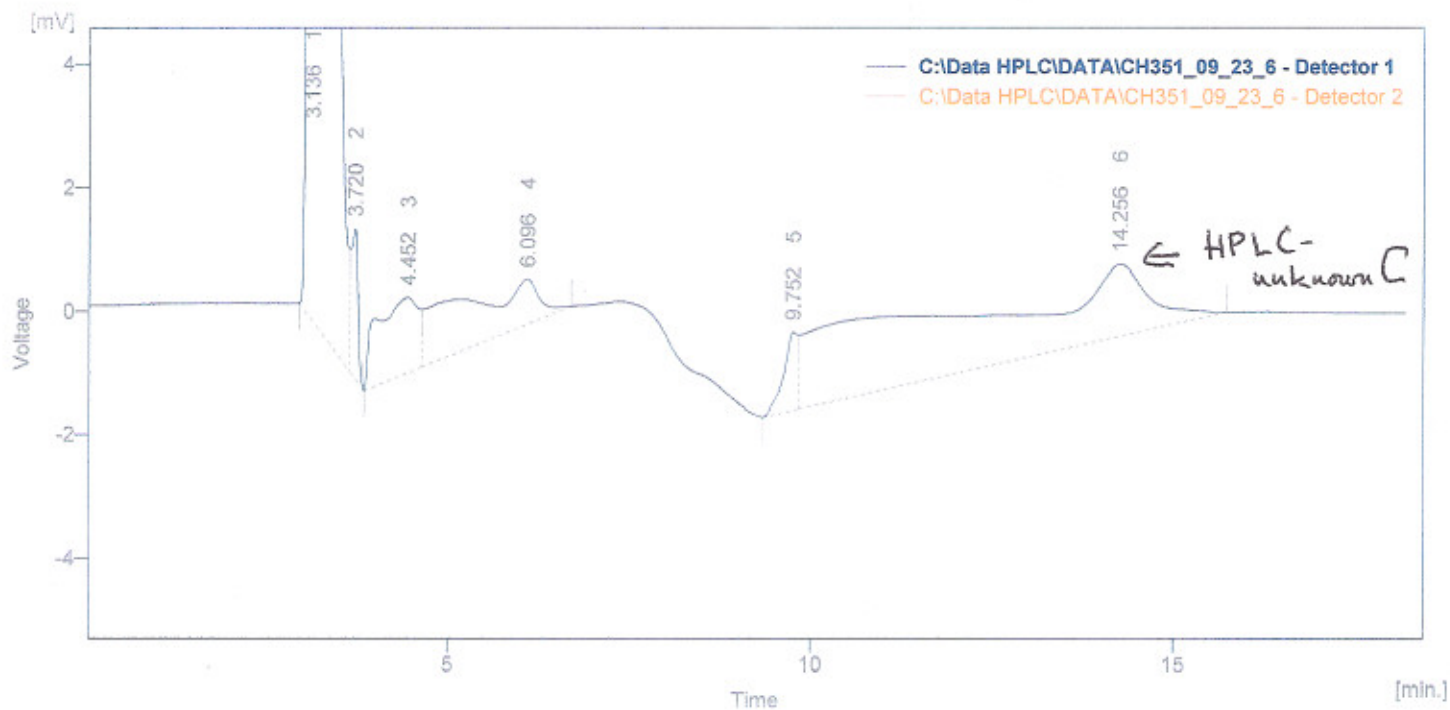


Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_6 - Detector 1)

|   | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%] | Height [%] | W05 [min] |
|---|-------------------|-------------|-------------|----------|------------|-----------|
| 1 | 3.136             | 414.919     | 18.253      | 48.5     | 72.8       | 0.39      |
| 2 | 3.720             | 16.021      | 2.436       | 1.9      | 9.7        | 0.11      |
| 3 | 4.452             | 48.643      | 1.219       | 5.7      | 4.9        | 0.73      |
| 4 | 6.096             | 71.863      | 0.729       | 8.4      | 2.9        | 0.44      |
| 5 | 9.752             | 17.761      | 1.267       | 2.1      | 5.1        | 0.21      |
| 6 | 14.256            | 286.510     | 1.189       | 33.5     | 4.7        | 0.86      |
|   | Total             | 855.718     | 25.072      | 100.0    | 100.0      |           |


Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_6 - Detector 2)

|   | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%] | Height [%] | W05 [min] |
|---|-------------------|-------------|-------------|----------|------------|-----------|
| 1 | 3.404             | 6814.679    | 1069.112    | 93.5     | 96.0       | 0.10      |
| 2 | 14.560            | 457.968     | 43.418      | 6.3      | 3.9        | 0.13      |
| 3 | 16.284            | 14.709      | 0.944       | 0.2      | 0.1        | 0.20      |
|   | Total             | 7287.356    | 1113.473    | 100.0    | 100.0      |           |

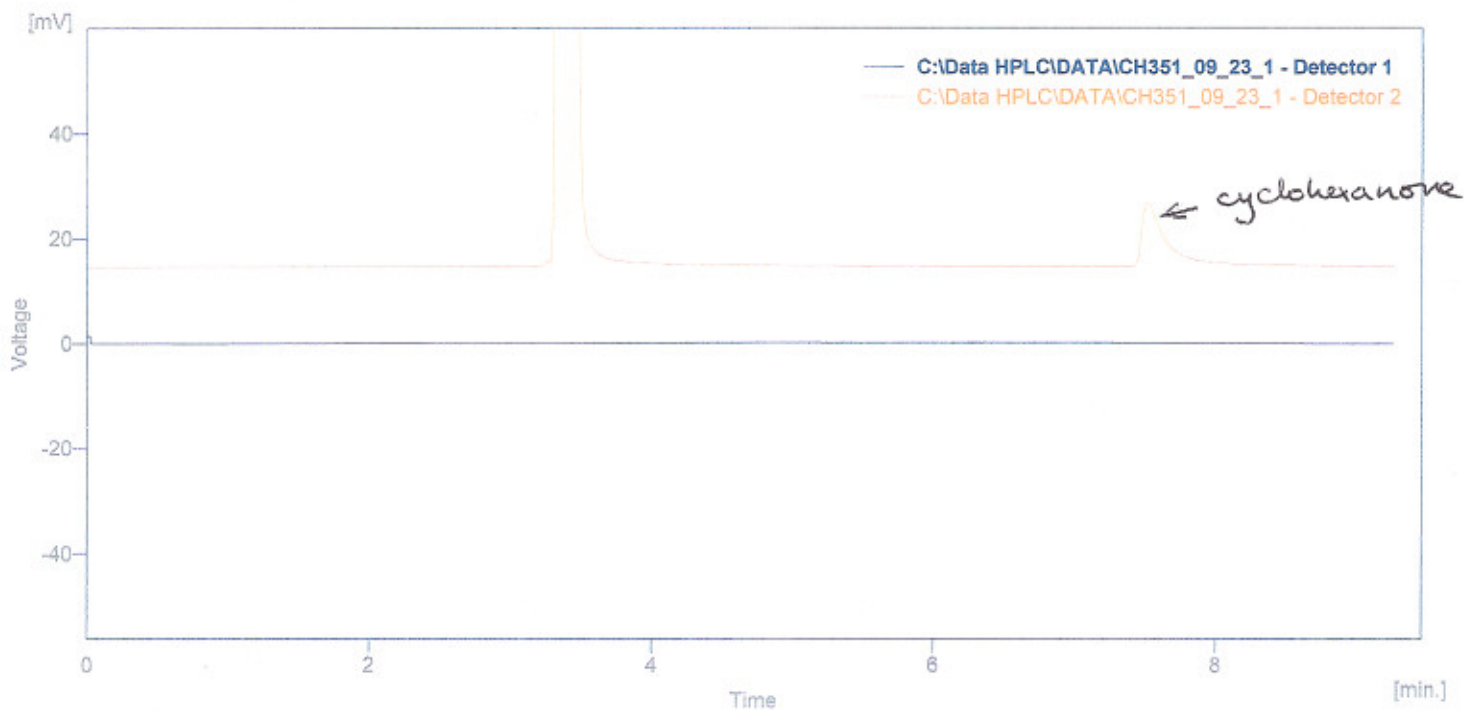

Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_1 - Detector 2)

|   | Reten. Time<br>[min] | Area<br>[mV.s] | Height<br>[mV] | Area<br>[%] | Height<br>[%] | W05<br>[min] |
|---|----------------------|----------------|----------------|-------------|---------------|--------------|
| 1 | 3.412                | 6088.089       | 1089.209       | 97.7        | 98.9          | 0.08         |
| 2 | 7.512                | 140.813        | 11.923         | 2.3         | 1.1           | 0.15         |
|   | Total                | 6228.901       | 1081.133       | 100.0       | 100.0         |              |

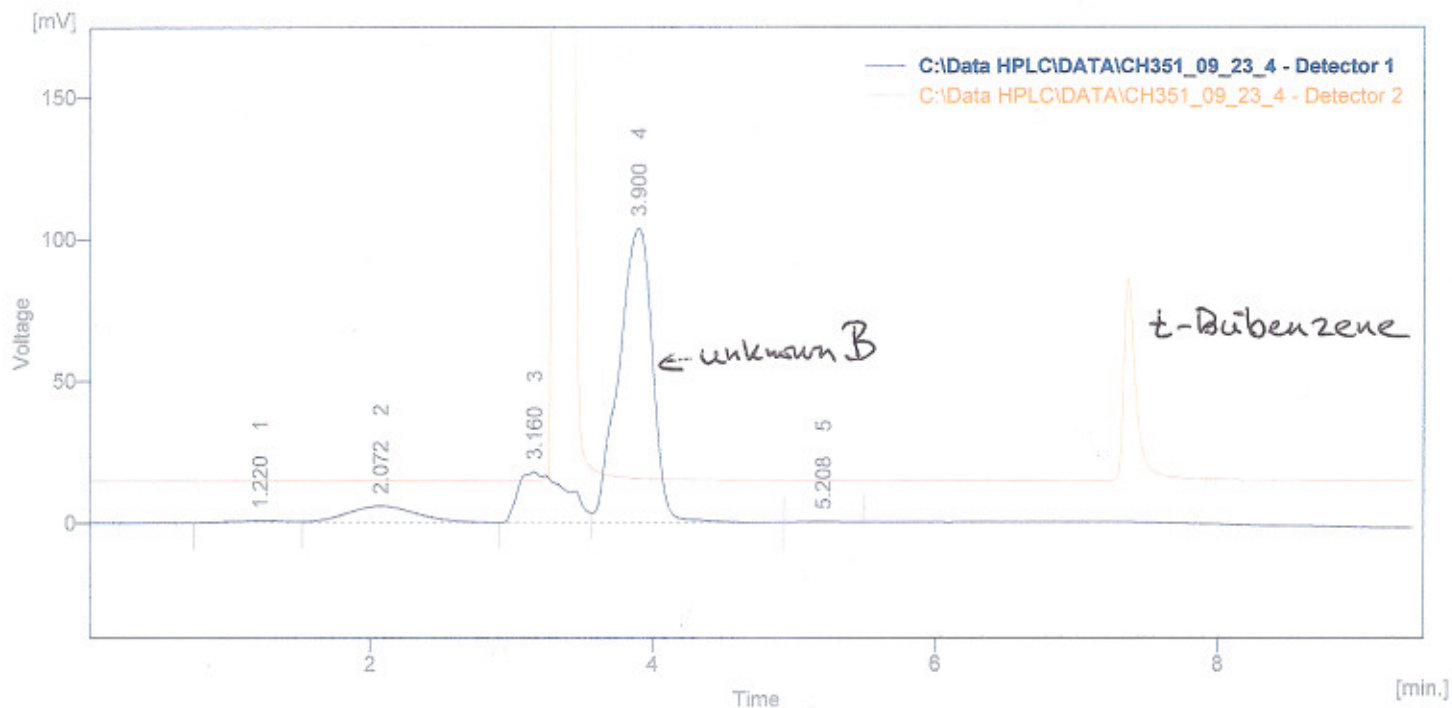


Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_4 - Detector 1)

|       | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%] | Height [%] | W05 [min] |
|-------|-------------------|-------------|-------------|----------|------------|-----------|
| 1     | 1.220             | 19.441      | 0.693       | 0.8      | 0.5        | 0.52      |
| 2     | 2.072             | 203.708     | 5.853       | 8.6      | 4.6        | 0.54      |
| 3     | 3.160             | 430.605     | 17.940      | 18.2     | 14.0       | 0.46      |
| 4     | 3.900             | 1715.302    | 103.608     | 72.3     | 80.7       | 0.26      |
| 5     | 5.208             | 3.384       | 0.228       | 0.1      | 0.2        | 0.25      |
| Total |                   | 2372.441    | 128.321     | 100.0    | 100.0      |           |

Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_4 - Detector 2)

|       | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%] | Height [%] | W05 [min] |
|-------|-------------------|-------------|-------------|----------|------------|-----------|
| 1     | 3.312             | 3577.716    | 1069.155    | 38.0     | 48.4       | 0.06      |
| 2     | 3.392             | 5408.604    | 1069.162    | 57.4     | 48.4       | 0.08      |
| 3     | 7.364             | 432.875     | 71.043      | 4.6      | 3.2        | 0.09      |
| Total |                   | 9419.195    | 2209.360    | 100.0    | 100.0      |           |



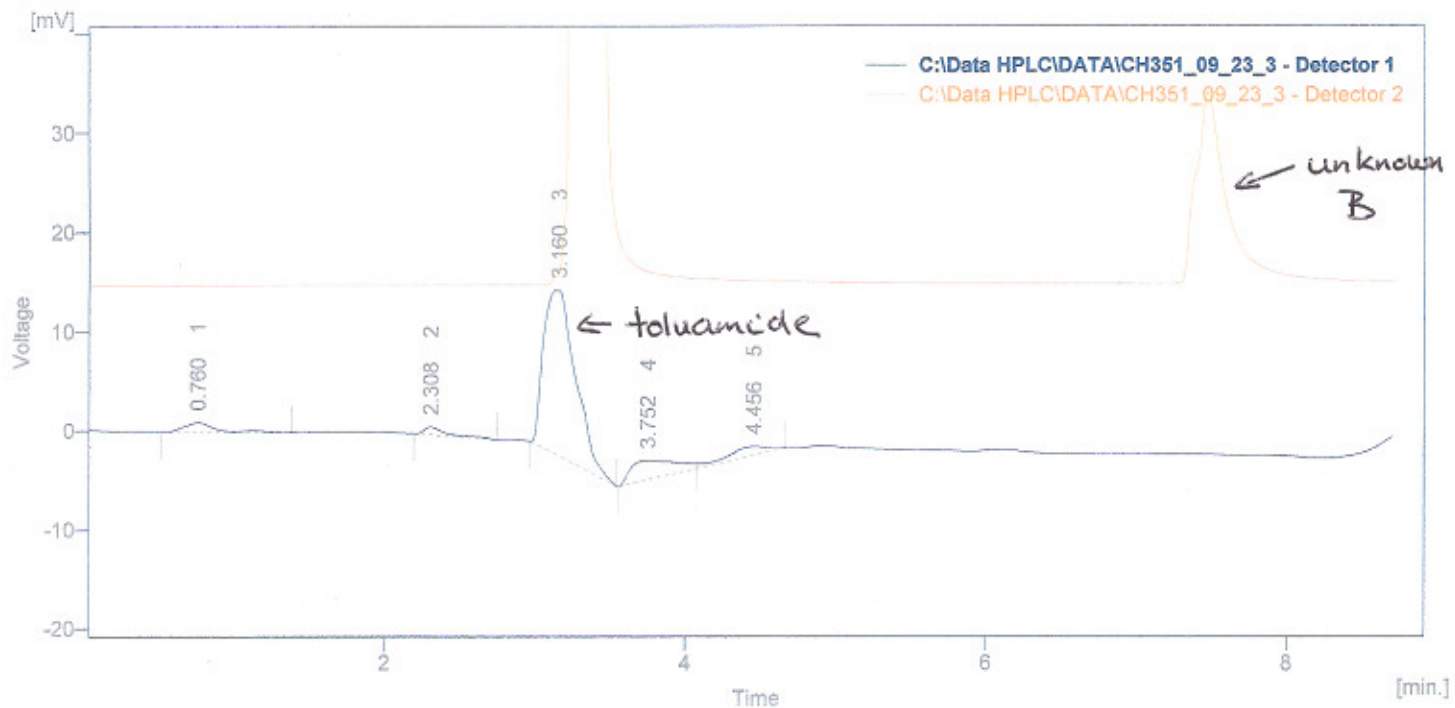


Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_3 - Detector 1)

|   | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%] | Height [%] | W05 [min] |
|---|-------------------|-------------|-------------|----------|------------|-----------|
| 1 | 0.760             | 14.711      | 0.954       | 4.5      | 4.5        | 0.21      |
| 2 | 2.308             | 8.433       | 0.790       | 2.6      | 3.7        | 0.12      |
| 3 | 3.160             | 246.821     | 16.712      | 75.2     | 78.6       | 0.23      |
| 4 | 3.752             | 39.724      | 1.933       | 12.1     | 9.1        | 0.45      |
| 5 | 4.456             | 18.411      | 0.875       | 5.6      | 4.1        | 0.33      |
|   | Total             | 328.100     | 21.264      | 100.0    | 100.0      |           |

Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_3 - Detector 2)

|   | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%] | Height [%] | W05 [min] |
|---|-------------------|-------------|-------------|----------|------------|-----------|
| 1 | 3.296             | 5879.287    | 1069.169    | 49.0     | 49.6       | 0.10      |
| 2 | 3.404             | 5845.444    | 1069.145    | 48.7     | 49.6       | 0.09      |
| 3 | 7.472             | 280.211     | 19.287      | 2.3      | 0.9        | 0.21      |
|   | Total             | 12004.942   | 2157.601    | 100.0    | 100.0      |           |

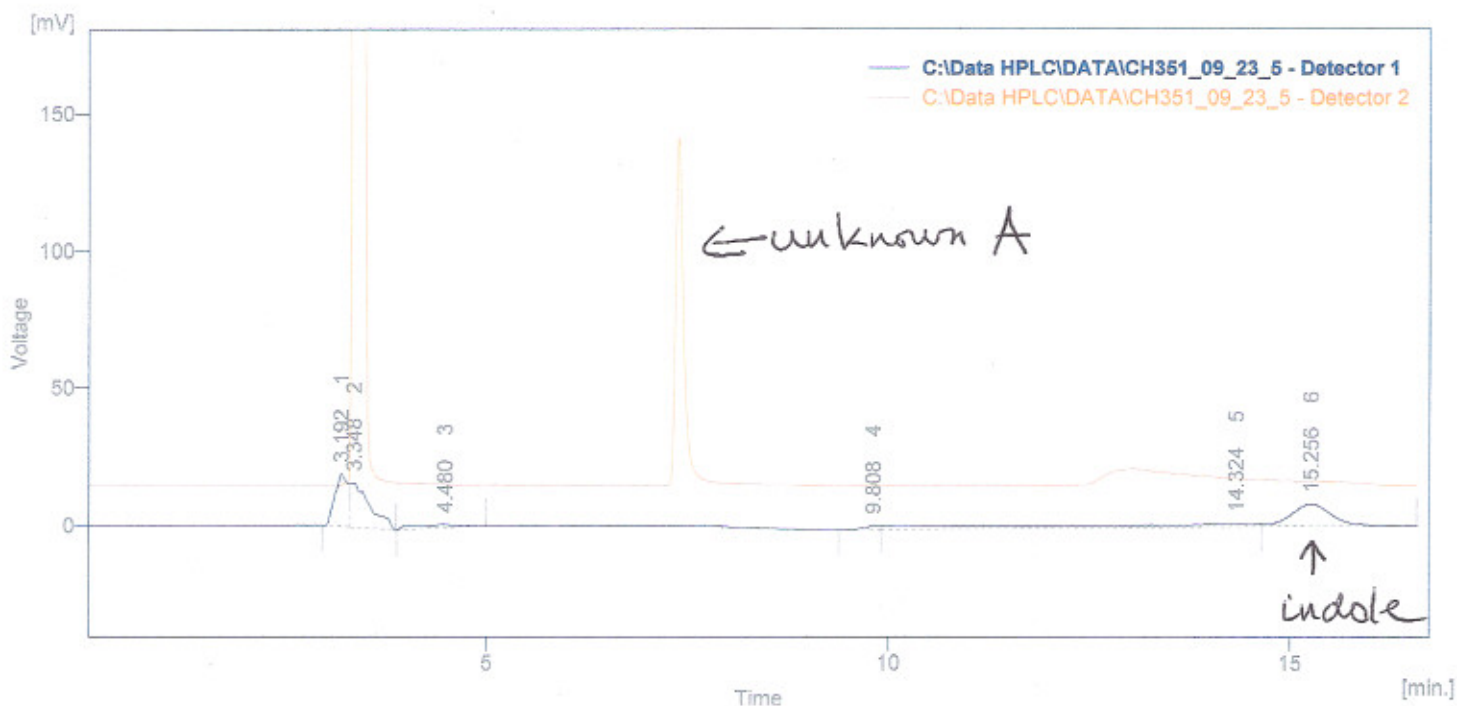


Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_5 - Detector 1)

|   | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%] | Height [%] | W05 [min] |
|---|-------------------|-------------|-------------|----------|------------|-----------|
| 1 | 3.192             | 214.096     | 19.053      | 18.1     | 41.0       | 0.20      |
| 2 | 3.348             | 276.844     | 16.084      | 24.7     | 34.6       | 0.25      |
| 3 | 4.480             | 48.603      | 0.951       | 4.3      | 2.0        | 1.02      |
| 4 | 9.808             | 18.949      | 1.269       | 1.7      | 2.8        | 0.21      |
| 5 | 14.324            | 285.875     | 1.108       | 25.5     | 2.4        | 0.86      |
| 6 | 15.256            | 275.998     | 7.958       | 24.6     | 17.1       | 0.52      |
|   | Total             | 1120.364    | 46.443      | 100.0    | 100.0      |           |

Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_5 - Detector 2)

|   | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%] | Height [%] | W05 [min] |
|---|-------------------|-------------|-------------|----------|------------|-----------|
| 1 | 3.420             | 9075.312    | 1069.156    | 85.9     | 89.0       | 0.14      |
| 2 | 7.380             | 916.206     | 126.227     | 8.7      | 10.5       | 0.10      |
| 3 | 13.044            | 568.226     | 5.915       | 5.4      | 0.5        | 1.34      |
|   | Total             | 10559.744   | 1201.299    | 100.0    | 100.0      |           |

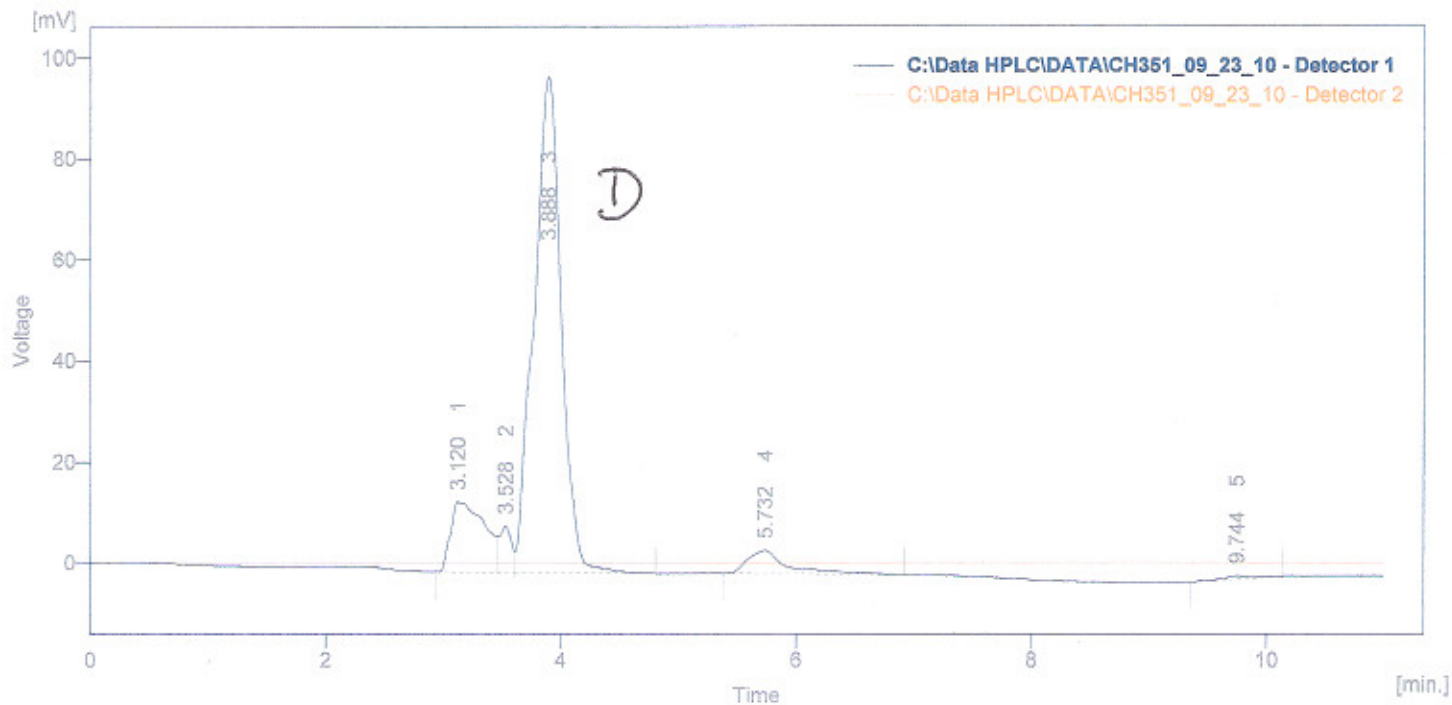

Result Table (Uncal - C:\Data HPLC\DATA\CH351\_09\_23\_10 - Detector 1)

|   | Reten. Time [min] | Area [mV.s] | Height [mV] | Area [%] | Height [%] | W05 [min] |
|---|-------------------|-------------|-------------|----------|------------|-----------|
| 1 | 3.120             | 279.793     | 13.917      | 13.6     | 11.0       | 0.41      |
| 2 | 3.528             | 65.919      | 9.183       | 3.2      | 7.3        | 0.14      |
| 3 | 3.888             | 1587.503    | 98.100      | 77.3     | 77.6       | 0.24      |
| 4 | 5.732             | 106.931     | 4.619       | 5.2      | 3.7        | 0.30      |
| 5 | 9.744             | 12.419      | 0.680       | 0.6      | 0.5        | 0.47      |
|   | Total             | 2052.568    | 128.498     | 100.0    | 100.0      |           |